


=====
Acq. Operator : Damir Seq. Line : 58
Acq. Instrument : Instrument 2 Location : Vial 56
Injection Date : 1/4/2023 9:14:54 AM Inj : 1
Inj Volume : 0.5 µl
Acq. Method : C:\CHEM32\2\DATA\CBX_GC2\2023_01_03_HHC_15MIN 2023-01-03 18-03-55\GC_2_HHC_FI_ BD.M
Last changed : 12/23/2022 4:51:54 PM by Damir
Analysis Method : C:\CHEM32\1\METHODS\GC_2_H4_CBD_FI_BD_23_01_20.M
Last changed : 1/22/2023 11:13:40 PM
(modified after loading)
Method Info : Metoda za terpene in CBX
Sample Info :

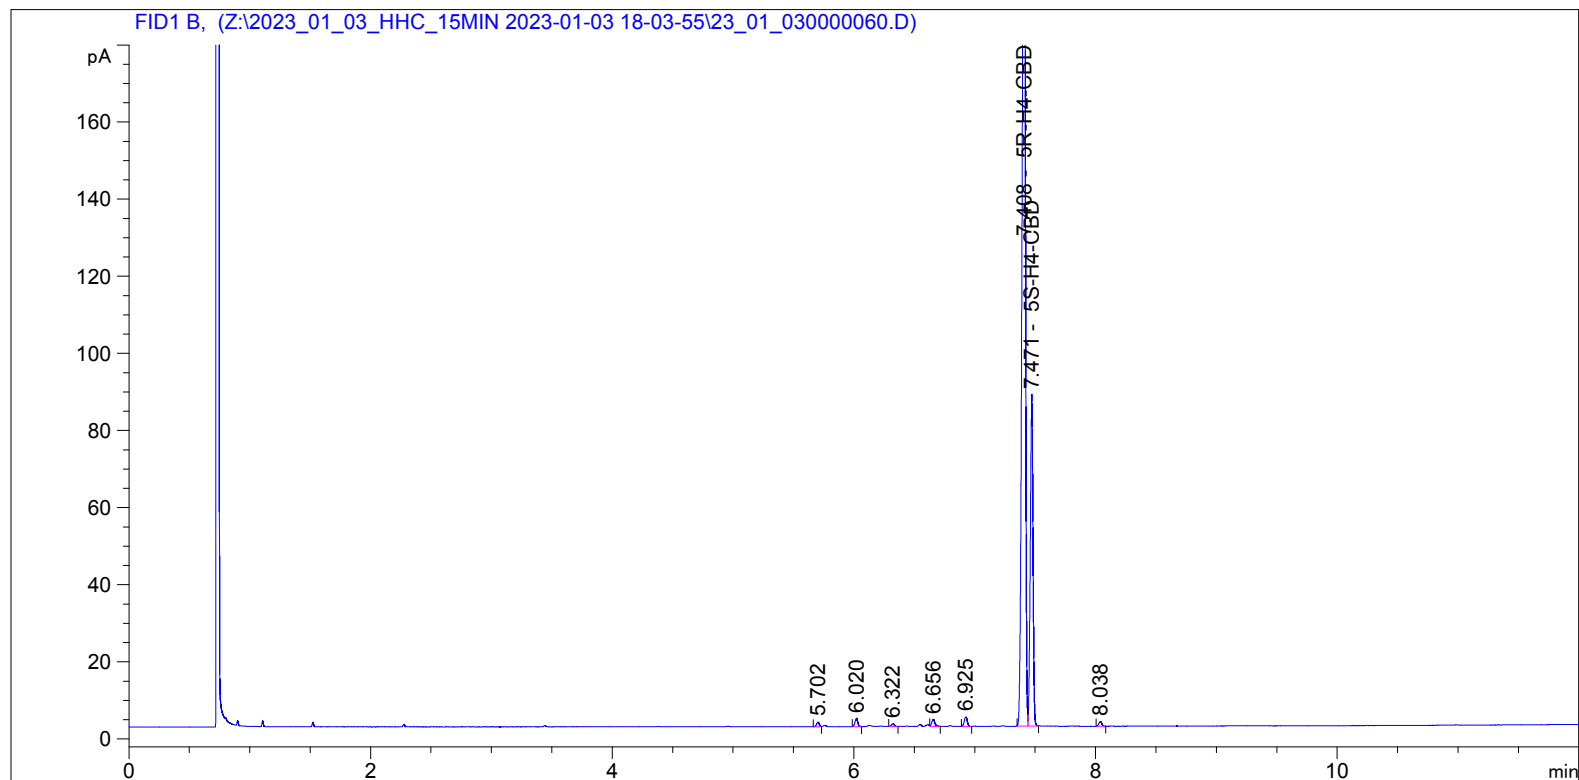

=====
Area Percent Report
=====

Sorted By : Signal
Calib. Data Modified : Sunday, January 22, 2023 11:13:39 PM
Multiplier: : 20.0000
Dilution: : 1.0000
Sample Amount: : 32.28000 [mg/ml] (not used in calc.)
Do not use Multiplier & Dilution Factor with ISTDs

Signal 1: FID1 B,

Peak #	RetTime [min]	Type	Width [min]	Area [pA*s]	Area %	Name
1	5.273		0.0000	0.00000	0.00000	Cannabidivarin, CBDV
2	5.702	BV	0.0253	1.80642	0.28586	?
3	5.802		0.0000	0.00000	0.00000	RT_13.14_M_314, CBT
4	5.870		0.0000	0.00000	0.00000	d9-THCV
5	6.020	BB	0.0247	3.38073	0.53500	?
6	6.322	BB	0.0253	1.16415	0.18423	?
7	6.530		0.0000	0.00000	0.00000	Cannabicyclol, CBL
8	6.656	VB	0.0289	3.46579	0.54846	?
9	6.925	BB	0.0277	4.28845	0.67864	?
10	6.997		0.0000	0.00000	0.00000	Cannabidiol, CBD
11	7.042		0.0000	0.00000	0.00000	Cannabichromene, CBC
12	7.235		0.0000	0.00000	0.00000	R-HHC
13	7.347		0.0000	0.00000	0.00000	S-HHC
14	7.408	BV	0.0300	481.14484	76.14081	5R-H4-CBD
15	7.471	VB	0.0247	134.63745	21.30628	5S-H4-CBD
16	7.582		0.0000	0.00000	0.00000	Cannabielsoin, CBE
17	7.635		0.0000	0.00000	0.00000	d8-THC
18	7.845		0.0000	0.00000	0.00000	d9-Dronabinol, d9-THC
19	8.038	BB	0.0249	2.02667	0.32072	?
20	8.326		0.0000	0.00000	0.00000	Cannabigerol, CBG
21	8.420		0.0000	0.00000	0.00000	Cannabinol, CBN
22	8.582		0.0000	0.00000	0.00000	M_344
23	8.711		0.0000	0.00000	0.00000	DVA 342 in 344
24	8.798		0.0000	0.00000	0.00000	CBDP
25	8.872		0.0000	0.00000	0.00000	DVA 342 in 344
26	9.038		0.0000	0.00000	0.00000	R-HHCP M_344
27	9.151		0.0000	0.00000	0.00000	S-HHCP M_344
28	9.237		0.0000	0.00000	0.00000	M_346
29	9.426		0.0000	0.00000	0.00000	M_342
30	9.606		0.0000	0.00000	0.00000	d9-THCP

Totals : 631.91450

2 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

*** End of Report ***